



OWH80 Series Single-Channel Programmable DC Power Supply Quick Guide

For product support, visit: www.owon.com.hk/download

※: The illustrations, interface, icons and characters in the user manual may be slightly different from the actual product. Please refer to the actual product.

Aug. 2025 edition V1.0.0

Copyright © LILLIPUT Company. All rights reserved.

The LILLIPUT's products are under the protection of the patent rights, including ones which have already obtained the patent rights and those which are applying for. The information in this manual will replace all materials published.

The information in this manual was correct at the time of printing. However, LILLIPUT will continue to improve products and reserves the rights to change specification at any time without notice.

owon[®] is the registered trademark of the LILLIPUT Company.

Fujian LILLIPUT Optoelectronics Technology Co.,Ltd.

No. 19, Heming Road

Lantian Industrial Zone, Zhangzhou 363005 P.R. China

Tel: +86-596-2130430

Fax: +86-596-2109272

Web: www.owon.com

E-mail: info@owon.com.cn

General Warranty

We warrant that the product will be free from defects in materials and workmanship for a period of 2 years from the date of purchase of the product by the original purchaser from our company. The warranty period for accessories such as probes, battery is 12 months. This warranty only applies to the original purchaser and is not transferable to a third party.

If the product proves defective during the warranty period, we will either repair the defective product without charge for parts and labour, or will provide a replacement in exchange for the defective product. Parts, modules and replacement products used by our company for warranty work may be new or reconditioned like new. All replaced parts, modules and products become the property of our company.

In order to obtain service under this warranty, the customer must notify our company of the defect before the expiration of the warranty period. Customer shall be responsible for packaging and shipping the defective product to the designated service centre, a copy of the customers proof of purchase is also required.

This warranty shall not apply to any defect, failure or damage caused by improper use or improper or inadequate maintenance and care. We shall not be obligated to furnish service under this warranty a) to repair damage resulting from attempts by personnel other than our company representatives to install, repair or service the product; b) to repair damage resulting from improper use or connection to incompatible equipment; c) to repair any damage or malfunction caused by the use of not our supplies; or d) to service a product that has been modified or integrated with other products when the effect of such modification or integration increases the time or difficulty of servicing the product.

Please contact the nearest Sales and Service Offices for services.

Excepting the after-sales services provided in this summary or the applicable warranty statements, we will not offer any guarantee for maintenance definitely declared or hinted, including but not limited to the implied guarantee for marketability and special-purpose acceptability. We should not take any responsibilities for any indirect, special or consequent damages.

Table of Contents

1. General Safety Requirement.....	1
2. Safety Terms and Symbols.....	3
3. Quick Start.....	4
3.1 Front Panel and Interface.....	4
3.1.1 Front Panel.....	4
3.1.2 Rear Panel.....	6
3.1.3 User Interface.....	7
3.2 General Inspection.....	8
3.3 Power-on Inspection.....	8
3.4 Output Inspection.....	9
3.4.1 Voltage Output Inspection.....	9
3.4.2 Current Output Inspection.....	9
4. PC software introduction.....	11
5. Troubleshooting.....	12
6. Appendix.....	13
6.1 Appendix A: Accessories.....	13
6.2 Appendix B: General Care and Cleaning.....	13

1. General Safety Requirement

Before any operations, please read the following safety precautions to avoid any possible bodily injury and prevent this product or any other products connected from damage. In order to avoid any contingent danger, this product is only used within the range specified.

Only the qualified technicians can implement the maintenance.

To avoid Fire or Personal Injury:

Use Proper Power Cord. Use only the power cord supplied with the product and certified to use in your country.

Product Grounded. This instrument is grounded through the power cord grounding conductor. To avoid electric shock, the grounding conductor must be grounded. The product must be grounded properly before any connection with its input or output terminal.

Limit operation to the specified measurement category, voltage, or amperage ratings.

Check all Terminal Ratings. To avoid fire or shock hazard, check all ratings and markers on the instrument. Refer to the user's manual for more information about ratings before connecting the instrument. Do not exceed any of ratings defined in the following section.

Do not operate without covers. Do not operate the instrument with covers or panels removed.

Use Proper Fuse. Use only the specified type and rating fuse for this instrument.

Avoid exposed circuit. Do not touch exposed junctions and components when the instrument is powered.

Do not operate if in any doubt. If you suspect damage occurs to the instrument, have it inspected by qualified service personnel before further operations.

Use your instrument in a well-ventilated area. Inadequate ventilation may cause an increasing of temperature or damages to the instrument. Please keep the instrument well ventilated, and inspect the air outlet and the fan regularly.

Do not operate in wet conditions. To avoid short circuit inside the

instrument or electric shock, never operate the instrument in a humid environment.


Do not operate in an explosive atmosphere. In order to avoid damages to the device or personal injuries, it is important to operate the device away from an explosive atmosphere.


Keep instrument surfaces clean and dry. To avoid the influence of dust or moisture in air, please keep the surface of device clean and dry.

2. Safety Terms and Symbols

Safety Terms

Terms in this Manual. The following terms may appear in this manual:

 **Warning:** Warning indicates the conditions or practices that could result in injury or loss of life.

 **Caution:** Caution indicates the conditions or practices that could result in damage to this product or other property.

Terms on the Product. The following terms may appear on this product:

Danger: It indicates an injury or hazard may immediately happen.

Warning: It indicates an injury or hazard may be accessible potentially.


Caution: It indicates a potential damage to the instrument or other property might occur.

Safety Symbols

Symbols on the Product. The following symbol may appear on the product:

 Hazardous Voltage

 Refer to Manual

 Protective Earth Terminal

 Chassis Ground

 Public Ground

3. Quick Start

3.1 Front Panel and Interface

3.1.1 Front Panel

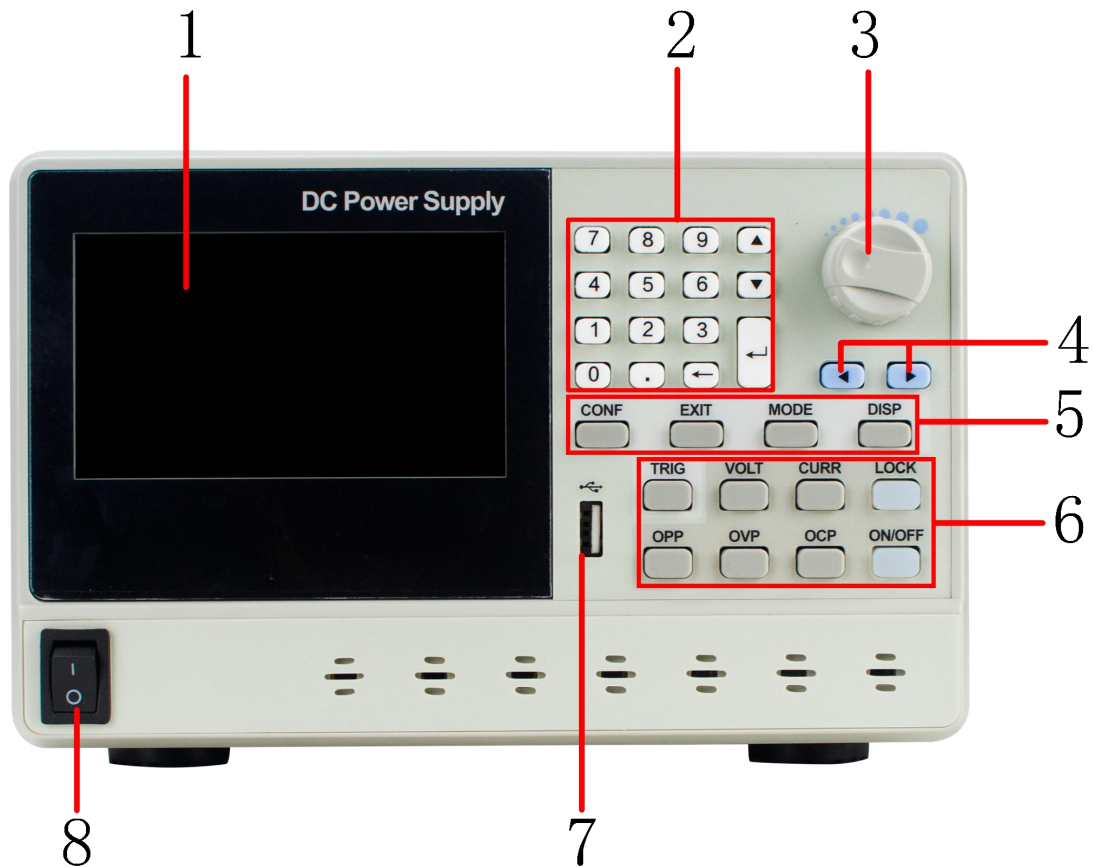


Figure 3- 1 Front panel overview

1	Display Screen	TFT color display showing output settings and real-time measurement values.
2	0-9 and . ← ↵	Numeric and decimal input keys for data entry. ←: Navigation key to cancel current operation or return to the previous screen. ↵: Confirms parameter input.
3	Rotary Knob	Allows users to scroll through options or adjust numerical values during parameter setting.

4	< >	Used to move the cursor left or right to the desired digit or parameter position.
5	System Function Keys	<ul style="list-style-type: none"> ● CONF: Opens the configuration page for system function settings. ● EXIT: Exits to the previous screen. ● MODE: Quick access to operation mode selection. ● DISP: Switches between numerical output display and waveform display.
6	Function Keys	<ul style="list-style-type: none"> ● TRIG: Manual trigger function. ● VOLT: Voltage setting key; press to enter voltage setting mode and adjust using numeric keys or rotary knob. ● CURR: Current setting key; press to enter current setting mode and adjust using numeric keys or rotary knob. ● LOCK: Locks all buttons and the rotary knob; press and hold to unlock. ● OPP: Over Power Protection setting. ● OVP: Over Voltage Protection setting. ● OCP: Over Current Protection setting. ● ON/OFF: Toggles output state (ON or OFF).
7	USB	USB data interface for communication or firmware update.
8	Power Switch	Mechanical switch to power the device ON or OFF.

3.1.2 Rear Panel

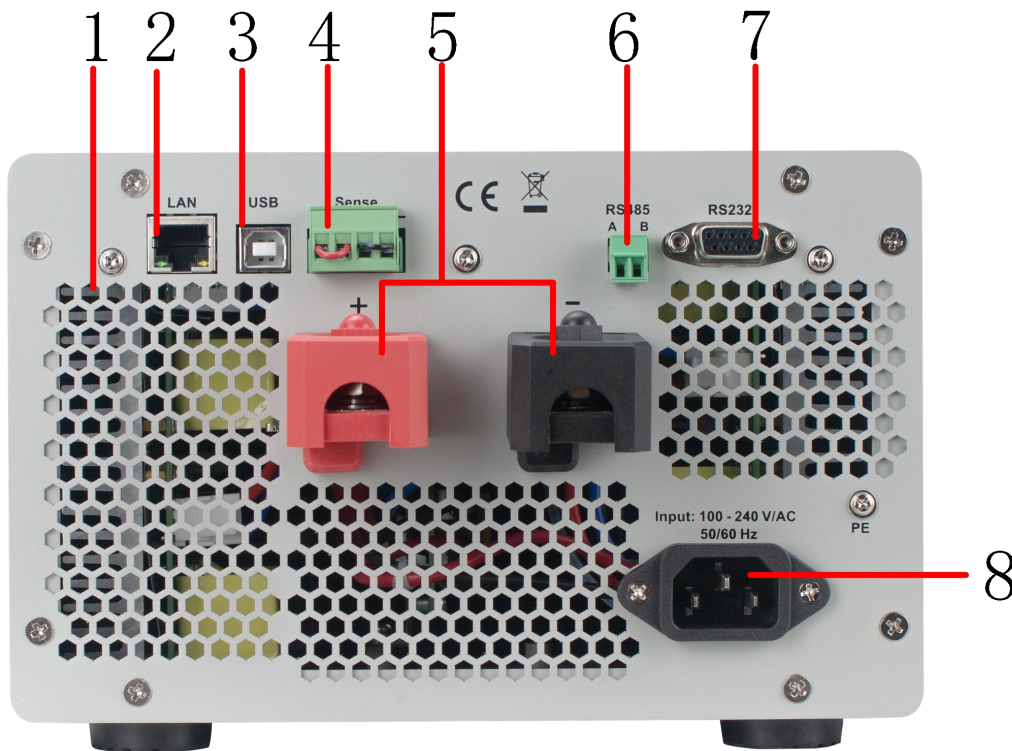


Figure 3-2 Rear panel overview

<p>1 Fan Air Outlet</p>	<p>Do not block the air outlet. Obstruction may cause inadequate internal cooling, leading to overheating and potential damage.</p>
<p>2 LAN Port</p>	<p>Ethernet communication interface for remote control. Connects the unit to a PC or network for remote operation.</p>
<p>3 USB Serial Port</p>	<p>USB communication port for connecting the device to a computer.</p>
<p>4 Remote Sense Terminals</p>	<p>Voltage sensing terminals used to compensate for voltage drop across output cables. Ensure Sense+ is connected to output +, and Sense- to output -. Do not reverse or leave the terminals open.</p>
<p>5 DC Output Terminal (+)</p>	<p>Positive output terminal for DC power delivery.</p>

6 RS-485 Interface	RS-485 communication port.
7 DB9 Port	DB9 serial interface supporting RS-232 communication protocol.
8 AC Power Input Terminal	AC input terminal for connecting the power cord to the device's input supply.

3.1.3 User Interface

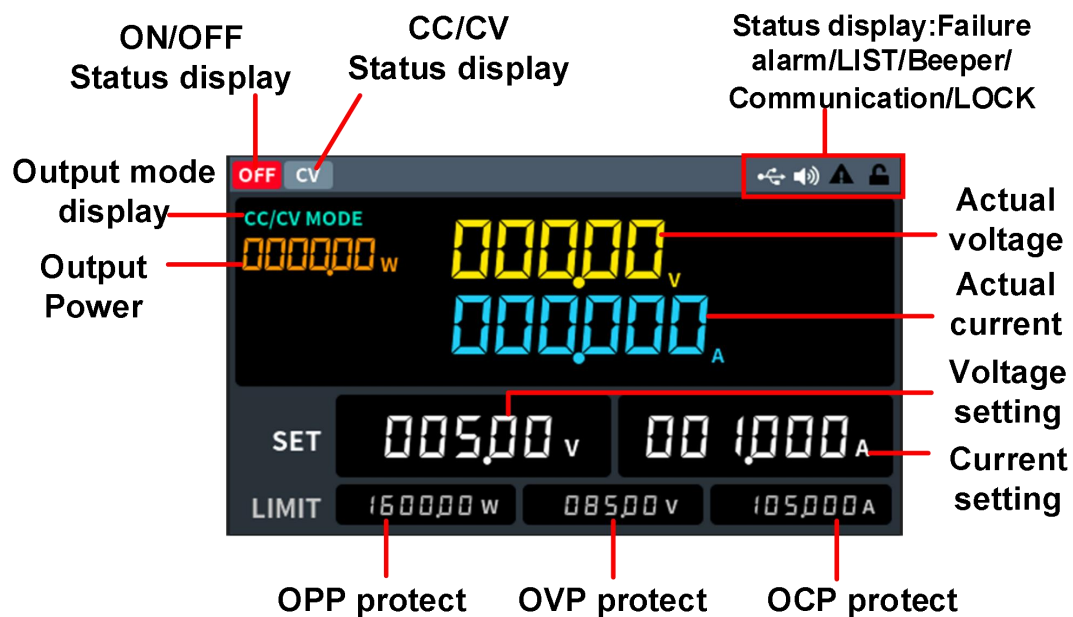








Figure 3-3 User interface

Status Icon

Icon	Description
	The panel keys are locked
	Panel USB data cable is transmitting
	Enable beeper
	Enable LIST function
	Record status
	A failure alarm

3.2 General Inspection

After you get a new DC power supply, it is recommended that you should make a check on the instrument according to the following steps:

1. Check whether there is any damage caused by transportation.

If it is found that the packaging carton or the foamed plastic protection cushion has suffered serious damage, do not throw it away first till the complete device and its accessories succeed in the electrical and mechanical property tests.

2. Check the Accessories.

The supplied accessories have been already described in Appendix A: Accessories of this manual. You can check whether there is any loss of accessories with reference to this description. If it is found that there is any accessory lost or damaged, please get in touch with our distributor responsible for this service or our local offices.

3. Check the Complete Instrument.

If it is found that there is damage on the first appearance of the instrument, or the instrument cannot work normally, or fails in the performance test, please get in touch with our distributor responsible for this business or our local offices. If there is damage to the instrument caused by the transportation, please keep the package. With the transportation department or our distributor responsible for this business informed about it, a repairing or replacement of the instrument will be arranged by us.

3.3 Power-on Inspection

- (1) Connect the instrument to an AC power source using the power cord supplied with the accessory.



Warning:

To prevent electric shock, make sure the instrument is properly grounded.

- (2) Press the **power button** on the front panel and the startup screen will be displayed on the screen.

3.4 Output Inspection

- (3) Output inspection is to ensure that the instrument can achieve its rated outputs and properly respond to operation from the front panel.



Warning:

Please verify the voltage withstand and polarity requirements of the instrument's output terminals and remote sensing connections. Do not reverse the +/- connections or exceed the rated output voltage, as improper operation may result in fatal injury or equipment damage.

3.4.1 Voltage Output Inspection

The following steps verify basic voltage functions without load:

- (1) When the instrument is under no load, select a channel and ensure the output current setting for this channel is not at zero.
- (2) Turn on the channel output, then ensure the channel is in Constant Voltage output mode.
- (3) Set some different voltage values on this channel; check if the actual voltage value displayed is close to the set voltage value, and also that the actual current value displayed is nearly to zero.
- (4) Check if the output voltage can be adjusted from zero to the maximum rating.

3.4.2 Current Output Inspection

The following steps check basic current functions to directly short the output two terminals:

- (1) Starting up.
- (2) Connect a short across (+) and (-) output terminals with an insulated test lead on this channel. Use a wire size sufficient to handle the maximum

current.

- (3) Set the output voltage to the maximum rating on this channel.
- (4) Turn on the channel output. Ensure the channel you used is in Constant Current output mode.
- (5) Set some different current values on this channel; check if the actual current value displayed is close to the set current value, and to check if the actual voltage value displayed is nearly zero.
- (6) Check that if the output current can be adjusted from zero to the maximum rating.
- (7) Turn off the channel output and remove the short circuit from the output terminals.

4. PC software introduction

1. Please go to the official website or contact your local dealer or our sales specialist to download or request the PC software.
2. Connect the USB CDC port on the back panel to the host computer. After the instrument is successfully connected, enter the mode setting to remotely operate the instrument.

Return Linking: OFF

Voltage **0.000V** Current **0.000A**

LIST MODE OFF

LIST Settings

List Load File Export(.CSV)

List Edit Current Cycle: 0 Mode: AUTO

Total Steps: 4 Cycle: 1

Del Add

	Voltage(V) (0-81.00)	Current(A) (0-31.000)	Time(S) (0.001-99999.999)
1	10	1	3
2	20	1	3
3	30	1	3
4	40	1	3

File List

File Import(.CSV)

file	path	time
------	------	------

File Selected Load

Protection OVP 65.00 V OCP 15.000 A
OPP 1200.00 W

5. Troubleshooting

1. The instrument is powered on but no display. Please following the steps:
 - Check if the power is connected properly.
 - Check if the fuse which is below the AC Power socket is used appropriately and in good condition (the cover can be pried open with a straight screwdriver).
 - Restart the instrument after the steps above.
 - If the problem still exists, please contact our customer service.

6. Appendix

6.1 Appendix A: Accessories

(The accessories subject to final delivery.)

Standard



Power Cord



User Manual



USB Cable

6.2 Appendix B: General Care and Cleaning

General Care

Do not store or leave the instrument where the liquid crystal display could be exposed to direct sunlight for long periods of time.

Caution: To avoid any damage to the instrument, do not exposed it to any sprays, liquids, or solvents.

Cleaning

Inspect the instrument as often as operating conditions require. To clean the instrument exterior, perform the following steps:

1. Wipe the dust from the instrument surface with a soft cloth. Take care not to scratch the transparent LCD protection screen when cleaning.
2. Disconnect power before cleaning your instrument. Clean the instrument with a damp soft cloth (not dripping with water). It is recommended to clean with soft detergent or fresh water. To avoid damage to the instrument, do not use any corrosive chemical cleaning agents.



Warning:

Before re-applying power, ensure that the instrument is completely dry, avoiding any electric shock or electrical short circuit resulting from moisture.
